


**XA**  
**AneuScore III**  
**(XA 13/18/21**  
**+ XA X/Y/18)**  
Aneusomy Probe

**Order No.:**  
D-5613-100-TC  
D-5613-500-TC

### Description

The XA AneuScore III Probe Kit contains different probe mixes, provided in separate test vials, for assessing chromosomal aneuploidies for chromosomes 13, 18, 21, X, and Y. The XA 13/18/21 mix of specific probes allows detecting copy number variations of chromosomes 13, 18, and 21. The green labeled probe hybridizes to a region at 13q14 including the RB1 locus, the blue (aqua) labeled probe hybridizes to a locus at 18q21, and the orange labeled probe hybridizes to a region at 21q22 including the DSCR4 (Down syndrome critical region 4).

The XA X/Y/18 mix of specific probes allows detecting copy number variations for chromosomes X, Y, and 18. The probe mix is composed of repetitive sequences which hybridize to the centromeric region of chromosomes X in green, Y in orange, and 18 in blue (aqua).

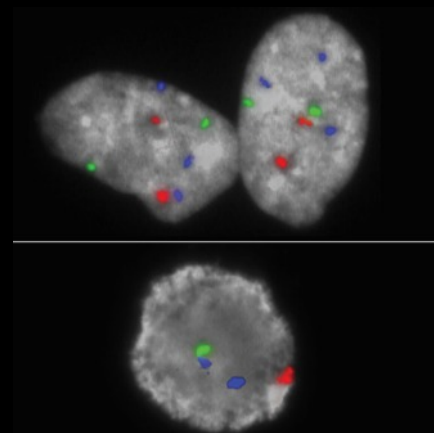

*XA AneuScore III hybridized to amniocytes of two different patients. XA 13/18/21 (upper image) shows a normal signal constellation for 13q14 and 21q22, two green and two orange signals, respectively. For the 18q21 locus-specific probe three blue signals are observed. XA X/Y/18 (lower image) shows a normal signal constellation with one orange (Y centromere-specific), one green (X centromere-specific) and two blue (18 centromere-specific) signals.*


### Clinical Details

Numerical aberrations of autosomes 13, 18, 21, and sex chromosomes X and Y account for about 95 % of birth defects in newborns. FISH applied to uncultured amniocytes provides a method to identify those aberrations much faster than conventional chromosome analysis. It has become a standard to provide preliminary results for the detection of anomalies in less than 12 hours.

#### Literature:

- Bryndorf et al (1996) Am J Hum Genet 59:918-926
- Tepperberg et al (2001) Prenat Diagn 21:293-301
- Stumm et al (2006) Cytogenet Genome Res 114:296-301

# FACTSHEET

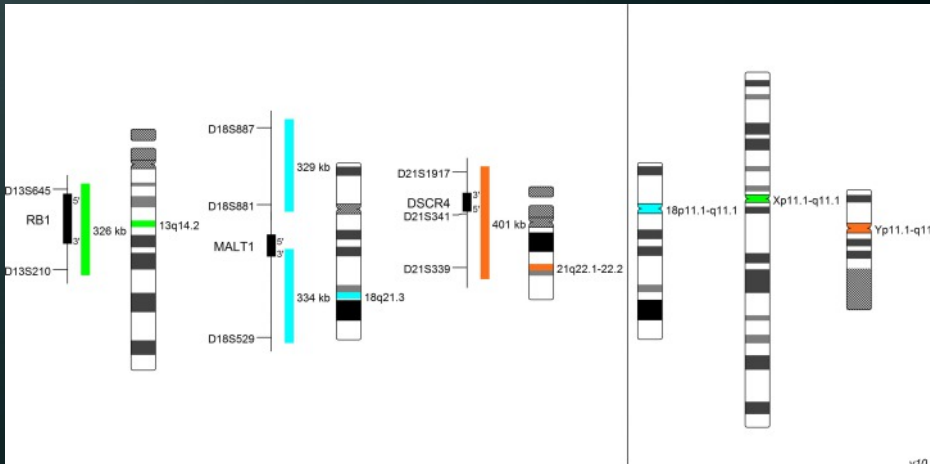

# MetaSystems Probes

## MetaSystems Probes GmbH (Headquarters)

1. Industriestrasse 7  
68804 Altlußheim, Germany  
tel +49 6205 2927 60 | fax +49 6205 2927 29  
info@metasystems-probes.com

## MetaSystems Group, Inc.

70 Bridge Street  
Newton, MA 02458, USA  
tel +1 6179 2499 50 | fax +1 6179 2499 54  
info@metasystems.org

## MetaSystems S.r.l.

Via Gallarate 80  
20151 Milano, Italy  
tel +39 0236 7587 51 | fax +39 0245 3753 03  
info@metasystems-italy.com

## MetaSystems India Pvt., Ltd.

No. 1/1, 1st Floor, 1st Main Rd., 2nd cross  
Thimmaiah Garden, R T Nagar  
Bangalore Karnataka, 560 032, India  
tel +91 9535 7788 01  
info@metasystems-india.com

## MetaSystems Asia Co., Ltd.

Unit 608, No. 12 Science Park West Avenue  
Hong Kong Science Park, Pak Shek Kok  
New Territories, Hong Kong  
tel +852 2587 8333 | fax +852 2587 8334  
info@metasystems-asia.com

## Related Products

Product	Size	Order No.
XA 21q22	100 µl	D-5601-100-OR
XA 13/21	100 µl	D-5602-100-OG
XA TriScore X/Y/21	100 µl	D-5603-100-TC
XA X/Y/18	100 µl	D-5606-100-TC
XA 13/18/21	100 µl	D-5607-100-TC
XA X/Y	100 µl	D-5608-100-OG
XA AneuScore I	100 µl	D-5604-100-TC
XA AneuScore II	100 µl	D-5609-100-TC

Document No. PFS-D5613-2018-05-01-S  
© 2018 by MetaSystems Probes

# FACTSHEET